

Sample Received: June 1, 2026

COA Issued: June 17, 2026

PRODUCT INFORMATION

Vendor:	Sample Name:	Sample Type:	Lot Number:	MW (g/mol):
EndoBiopeptides	Retatrutide 30mg	White lyophilized powder	RT30	4731.2


ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: Retatrutide	Retatrutide	MALDI-MS	✓ Conforms
Content	30.84 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.9%	RP-HPLC (214 nm)	✓ Conforms
Sterility	Not Detected	<USP71>	✓ Conforms
Heavy Metals	<0.01ppm	<USP232>	✓ Conforms
Endotoxin	<0.05 EU/mL	<USP85>	✓ Conforms

HPLC Chromatogram (Retention Time: 11.044 min)

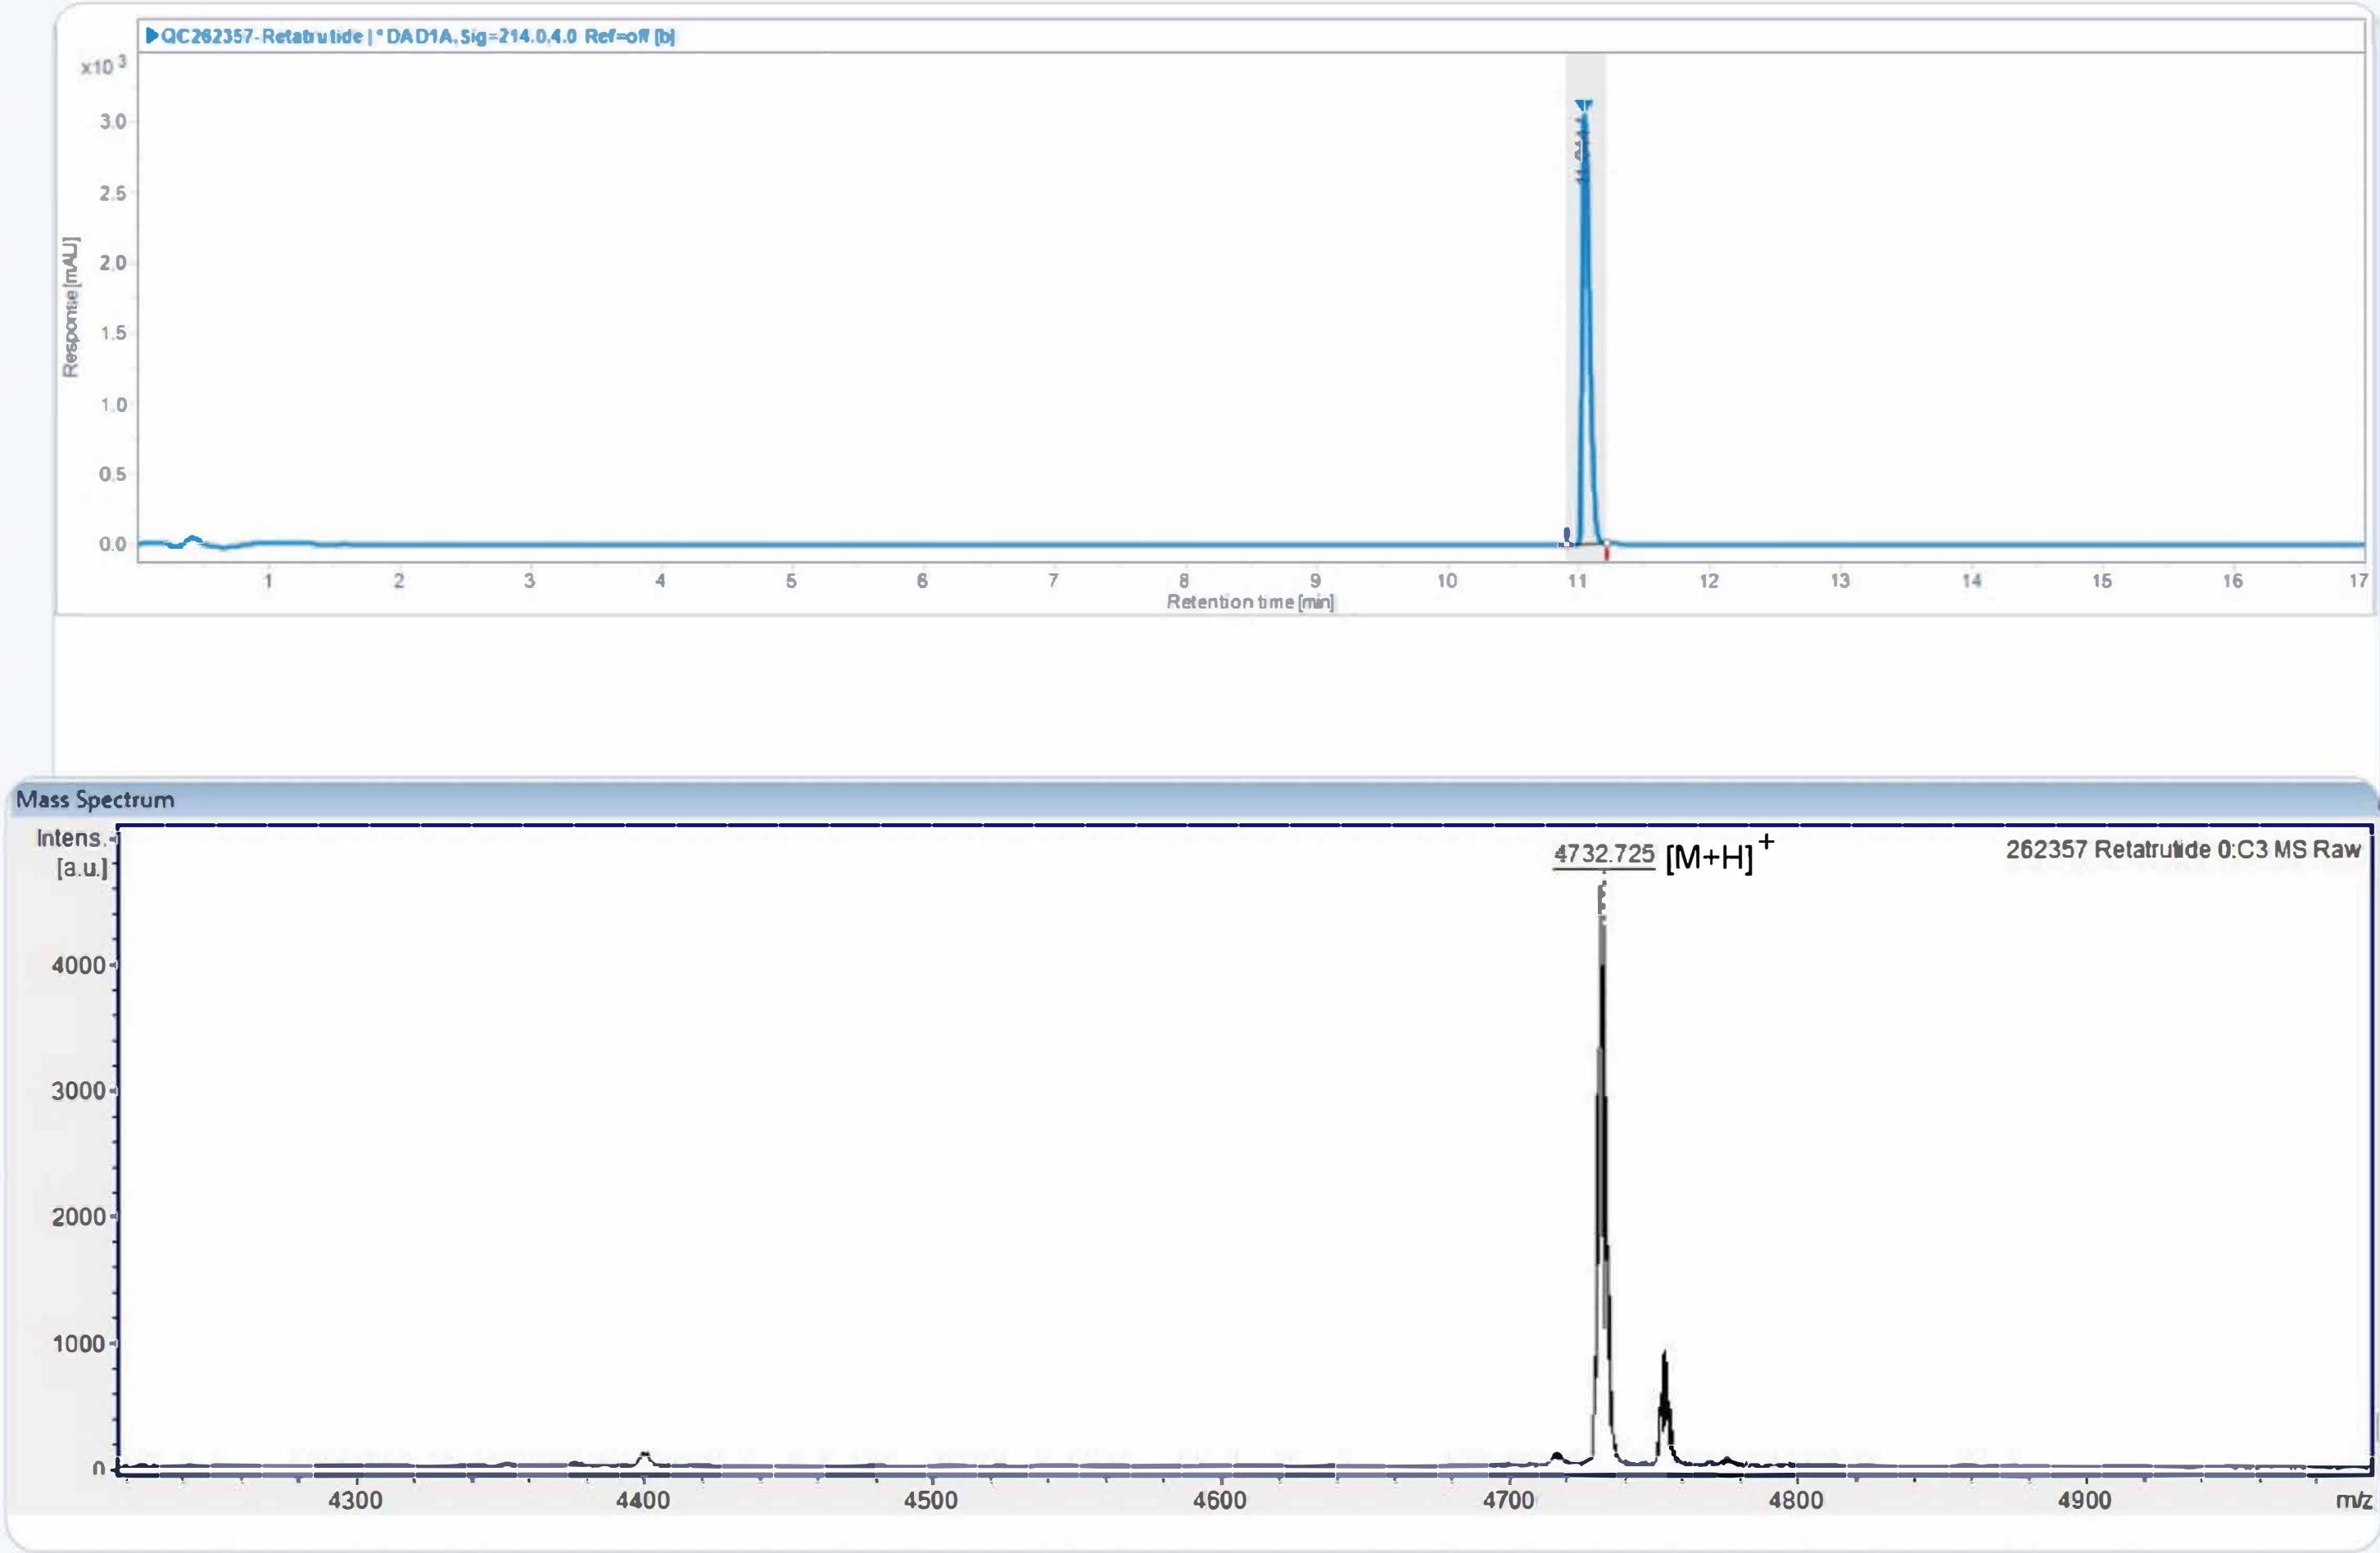

Certification: This COA confirms that the tested material meets or exceeds WEIPU’S analytical quality specifications for peptide research use.



Shane Straight

Shane Straight, M.S.